
# **POCKET HANDLE**



PLEASE READ AND FOLLOW THESE INSTRUCTIONS CAREFULLY



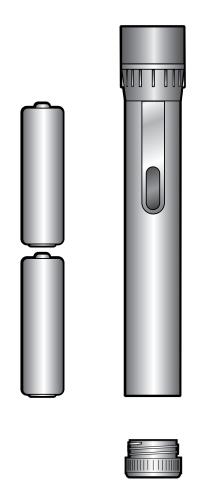

#### Connection of the instrument heads to the handle.

The connection between the instrument head to the handle is a screw thread. To connect our instrument head connect as shown and rotate in clockwise direction. Ensure the connection between the head and handle is positive.



#### Compatibility

The Keeler Specialist, Professional, Standard and Practitioner Ophthalmoscopes and Keeler Retinoscopes are compatible with Keeler Vista 2.8v and 3.6v Keeler handles.



## On/Off brightness control

To switch the instrument on, rotate the brightness control as indicated to the right.

To switch off the instrument, rotate the brightness control as indicated to the left.

## **Inserting/Replacing Batteries**

Unscrew battery cap, insert batteries and replace battery cap as shown. The following dry cell batteries should be used:

**Keeler Pocket handle** – 2 x 1.5v AA size batteries. – Duracell MN 1500 or equivalent.

### Cleaning Instructions

Only manual non-immersion cleaning as described below should be used for the instrument:

- 1. Wipe the external surface with a clean absorbent, non shedding cloth dampened with a water / detergent solution (2% by volume) or water / isopropyl alcohol solution (70% by volume).
- 2. Ensure that excess solution does not enter the instrument. Use caution to ensure cloth is not saturated with solution.
- 3. Surfaces should be carefully hand-dried using a clean non-shedding cloth.
- 4. Safely dispose of used cleaning materials.

### **Warranty & Service**

No user serviceable parts - all preventative maintenance and servicing must only be performed by authorised Keeler representatives.

Your Keeler handle is guaranteed for 3 years and will be replaced or repaired free of charge subject to the following:

- 1. Any fault is due to faulty manufacture
- 2. Proof of purchase accompanies any claim.



#### MANUFACTURED IN THE UK BY:

## **Keeler Limited**

Clewer Hill Road Windsor Berkshire SL4 4AA England

Tel: +44 (0)1753 857177 Fax: +44 (0)1753 827145 FREEPHONE: 0800 521 251

Distributed by:

## **Keeler Instruments Inc**

456 Parkway Broomall PA 19008, USA

Toll Free: 1 800 523 5620

Tel: 610 353 4350 Fax: 610 353 7814

The CE mark on this 
product indicates it has 
been tested to and 
conforms with the 
provisions noted within 
the 93/42/eec Medical 
Device Directive.





Distributor

